VERIFICATION OF CALIBRATION REPORT
of DataMaster cdm Breath Test Instrument
State of Alaska

JAN 2 1 2010

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N _130290_

A

Supervisor/Operator Performing the Verification Procedure:

Name _STEVE DUNN_   ID# _4106_   Date _1-21-10_

Agency _APD_   Phone # _764-1361_

Instrument Location _ANCHORAGE JAIL_

B

Alco S/N _X301540_   Target Value _.085_   High Pressure _1050 PSI_

Alco Test Value Average _.085_   _.085_
1st Alco   2nd Alco

Signature _____ SD _____   CCB 1/22/10

(OVER)

(Do Not write in the area below)

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

(1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.

(2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.

(3) I am the Scientific Director of the State Breath Alcohol Program.

(4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.

(5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.

(6) The referenced instrument is certified for evidentiary use in the State of Alaska.

Nita J Bolz
Nita J. Bolz
Scientific Director
State Breath Alcohol Program

Subscribed and sworn before me this _10th_ day of _Feb_, 2010.

Carolyn Noland
(Notary Seal Stamp)
Carolyn M. Noland
Notary Public, State of Alaska
Commission Expires with Office

Carolyn M. Noland
NOTARY
PUBLIC
STATE OF ALASKA
State of Alaska

BT9 03/00

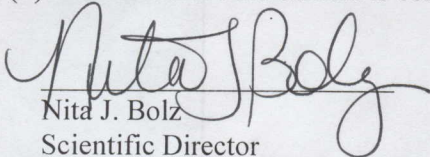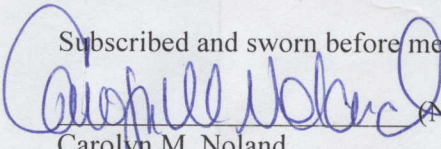# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument
State of Alaska
Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N __130290__ ✓

(CONTINUED FROM FRONT PAGE)

C	TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

S. Dunn #1361

```
ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130290 ✓

JANUARY 21, 2010          CAB 1/22/10

OPERATOR'S NAME:
  DUNN/S
OPERATOR'S NUMBER: 4106
SUBJECT'S LAST NAME:
  VERIFICATION OF CAL
SUBJECT'S FIRST NAME/MI :
  V
O.L. #: V
DEPT/AGENCY: ANC1
CASE/REPORT: V
TEST TYPE: V
ALCO TARGET VALUE: .085  ✓
ALCO S/N: X301540        ✓

  --- BREATH ANALYSIS ---

.085 ADJUSTED FOR 29.49 in
ALCO TARGET        .083      03:57
BLANK TEST         .000      03:58
INTERNAL STANDARD  VERIFIED  03:58
ALCO TV 29.49 in   .085  ✓   03:59
BLANK TEST         .000      03:59
SUBJECT SAMPLE CAB .000      04:00
                 1/22/10
BLANK TEST         .000      04:01
ALCO TV 29.49 in   .085  ✓   04:01
BLANK TEST         .000      04:02
```

DIAGNOSTIC CHECK

S. Dunn #1361

```
ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130290

JANUARY 21, 2010
TIME 03:55

  --- DIAGNOSTIC CHECK ---

COMPUTER:              OKAY

PROGRAM:               OKAY

SOFTWARE DATE:         01/08/09

HEATERS
SAMPLE CHAMBER:        49c
BREATH TUBE:           41c

BAROMETER:             29.49 in

FLOW DETECTOR:         OKAY

PUMP
HIGH SPEED:            OKAY

DETECTOR:              OKAY

FILTERS:               OKAY

QUARTZ STANDARD:       OKAY

CALIBRATION:           OKAY

      PRINTER TEST
!"#$%&'()*+,-./0123456789:;<=>?@ABCDEFG
HIJKLMNOPQRSTUVWXYZ[\]^_`abcdefghijklmno
pqrstuvwxyz{|}~
```

BT9 03/00